


Clinical Tests and Reports on BABY-COMP® and LADY-COMP®

... the safe
fertility computers
for over 25 years

LADY-COMP®
BABY-COMP®
pearly®

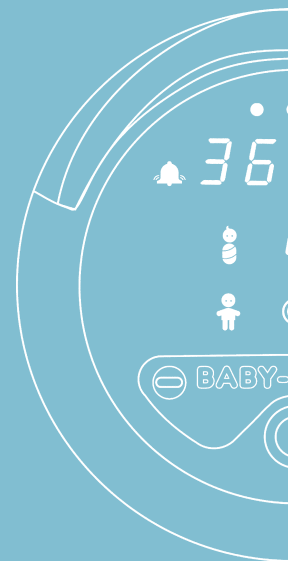

- 1. Medical Product, Directive 93/42/EEC, January, 2009**
Quality Management, Medical Device, Directive 93/42/EEC
Quality Management, Voluntary participation in regular monitoring EN ISO13485:2003 + AC:2007.
- 2. Medical Evaluation, Dr. Andreas Marx – ClevaMed, Sept. 20th, 2007**
EG-Instruction 93/42 EWG und MEDDEV.2.7.1
'very high degree in Method-Security, which clearly stands out from competitive devices'.
- 3. Certification EMV EN60601-1-2**
March 12th, 2007 LADY-COMP®
March 19th, 2007 BABY-COMP®
July 10th, 2007 pearly®
- 4. Certification of Production**
ISO9001: 2000 / ISO14001: 2004
Environmental Assessment Bavaria, December 16th, 2005
- 5. Congresso della Societa Italiana della Contraccezione, June 16-18th, 2005 Lettura BABY-COMP®**
Dr. Hubertus Rechberg: Contraception and Baby-planning with LADY-COMP® and BABY-COMP®
- 6. FDA, January 2005 Office of Device Evaluation (ODE)**
as an aid in ovulation prediction
- 7. New York Observer, Juni 25th, 2004**
Sheelah Kolhatkar: Orgasmatron shows up: High-Tech-Rhythm
- 8. Advances in Contraception 1998; 14: 97-108**
Prof. Freundl, Frank-Herrmann, Prof. Godehardt, Klemm, Bachhofer
Trial of contraceptive effectiveness of LADY-COMP® / BABY-COMP®
Results: User Pearl-Index 0.7.
- 9. Düsseldorf 1998, Dissertation Bachhofer, Prof. Freundl, Frank-Herrmann, Prof. Godehardt, Klemm**
686 women in more than two years use = Pearl-Index 0.7.
Field study in Switzerland, Germany and Mexico.
- 10. Sassari 1997, Prof. S. Dessole, Fadda, Rosas, Scapinelli, Inaudi, Ambrosini**
Test on women sterile for 3 – 8 years. BABY-COMP® compared with clinical testing.
Results: 100% match on luteal deficiency, anovulatory cycles and pregnancies.
Clinical found 86% Ovulation's, BABY-COMP® 80%. (Original in English)
- 11. Birmingham 1997, Prof. Freundl**
Test of 686 women over 24 month and 12.213 Cycles. *Results:* see below 8.
- 12. Erlangen 1994, Prof. Wildt**
Clinical testing and comparison with BABY-COMP®.
Results: perfect match between clinical findings and fertility indications of BABY-COMP®.
- 13. Fertilität 1992, Nr. 8, Pages 66-67**
Clinical testing compared with BABY-COMP® fertility indications.
Results: in no case BABY-COMP® missed the beginning of fertile time,
cycle disturbances were detected and treated right.
- 14. Amsterdam 1992, Prof. Martinez, v. Hoof, Schoute, v.d. Meer**
Clinical Test and research on Hormone- and Temperature shifts.
Results: They do correlate and there is BABY-COMP® that might improve reliability,
acceptability and application of BBT in fertility investigation. (Original in English)
- 15. Barcelona Congress 1992, Prof. Freundl, Bauer, Bremme, Döring, Frank-Herrmann**
Test on fertile women. Compared with clinical testing.
Definition: 6 Days are fertile.
Results: LADY-COMP® found temperature shift in each cycle. Number of fertile days 11.1 +/- 3.
Length of cycles 25-35. No pregnancy on 'green' days. (Original in English)
- 16. Rhodos 1988, Prof. Freundl, Frank-Herrmann, Toncaboni**
 - a) test on preciseness of temperature readings
Results: Temperature readings highly precise p2 0.01.
 - b) test on prevention compared with clinical testiness.
Results: no unwanted Pregnancies on 'green' days.
 - c) test on planing.
Results: 2 out of 5 conceived already during the test. (Original in English)



Quality Management
Medical Device
Directive 93/42/EEC



Quality Management
Voluntary participation in regular
monitoring
EN ISO 13485:2003 + AC:2007



VE Valley Electronics GmbH
Wengwies 2
D-82438 Eschenlohe
Germany

Tel (+49) 0 88 24 18 31
Fax (+49) 0 88 24 80 71

www.lady-comp.com
info@lady-comp.com

www.valley-electronics.com
info@valley-electronics.com